

# NASA TECH BRIEF




NASA Tech Briefs announce new technology derived from the U.S. space program. They are issued to encourage commercial application. Tech Briefs are available on a subscription basis from the National Technical Information Service, Springfield, Virginia 22151. Requests for individual copies or questions relating to the Tech Brief program may be directed to the Technology Utilization Office, NASA, Code KT, Washington, D.C. 20546.

## Automatic Optometer Operates with Infrared Test Pattern

### The problem:

To monitor the refractive strength of the human eye in order to study accommodation characteristics such as speed of response to changing views and maximum focusing power.

strength of the eye lens may be changing continually. Light reflected from the retina passes through the half-field stop  $S_2$  and the corneal-reflection stop to the photodetector; the photodetector signal contains 160 Hz component if the input image pattern is not in

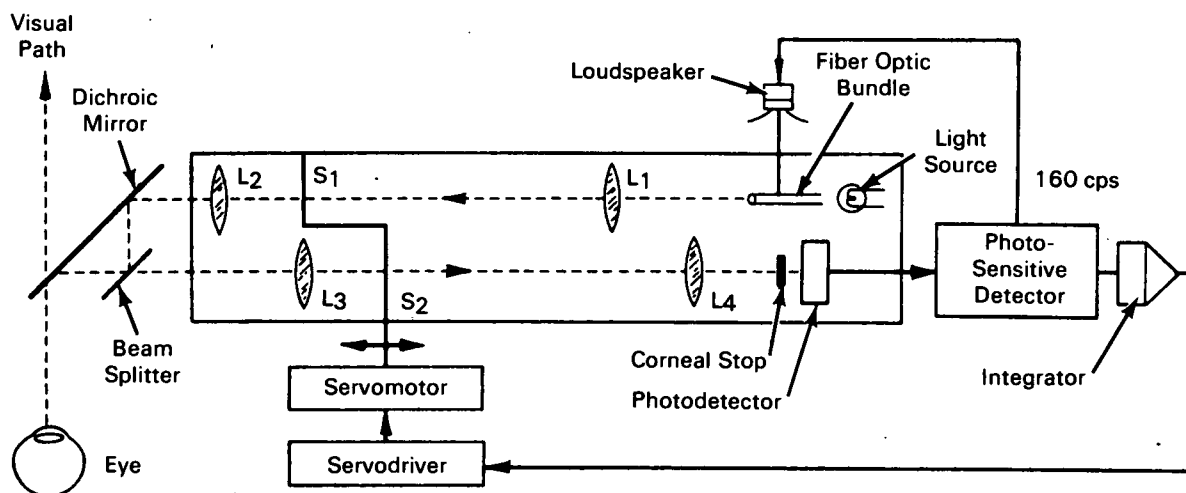

### The solution:

An optometer that automatically and continuously images an infrared test pattern onto the retina; the condition of focus of the eye at any instant is determined from the optometer settings needed to maintain focus of the pattern on the retina.

### How it's done:

Infrared light passing through a fiber optic bundle vibrating at about 160 Hz transverse to the image slit  $S_1$  forms a bar pattern which is maintained at focus on the retina by servocontrol, even though the refractive

focus on the retina. The photodetector signal is directed to a phase-sensitive detector which furnishes to the servodriver a dc signal of the polarity and magnitude required to cause the servomotor to move the bar image at  $S_1$  until there is a zero signal from the detector. The servomotor also controls the axial position of stop  $S_2$  through a mechanical linkage, maintaining it in the retinal image plane despite changes in the refractive strength of the eye. The integrator makes possible a zero position-error system.

The time between the onset of a visual target displacement and the beginning of the resultant change

(continued overleaf)

in accommodative strength can be measured by noting the time lapse between target displacement and initial motion of the servomotor. The rate of change of refractive strength of the eye can be measured from time plots of servomotor motions.

**Notes:**

1. Accommodation responses of five commercial airline pilots under 35 years of age were measured for 2-diopter displacements of a target. For a target moving toward infinity, pilot response times were less than 1.5 seconds, but for a target moving toward the subjects, response times varied from less than one to more than six seconds.
2. A related instrument is described in NASA Tech Brief 70-10568.

3. Requests for further information may be directed to:

Technology Utilization Officer  
Ames Research Center  
Moffett Field, California 94035  
Reference: TSP70-10401

**Patent status:**

Inquiries about obtaining rights for the commercial use of this invention may be made to NASA, Code GP, Washington, D.C. 20546.

Source: T. N. Cornsweet and H. D. Crane of  
Stanford Research Institute  
under contract to  
Ames Research Center  
(ARC-10095)